



PROCEDURE




1. Place the test tubes containing reagent R1 in one of the incubation cells and let them warm for at least 5 minutes.

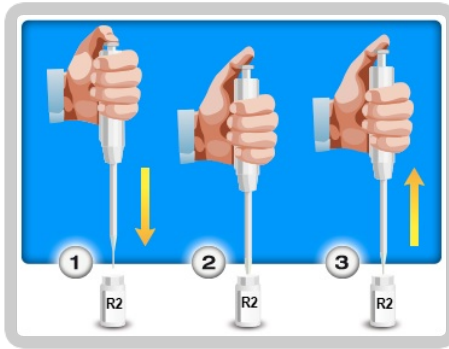

2. Collect 30 µL of R2 with the pipette.

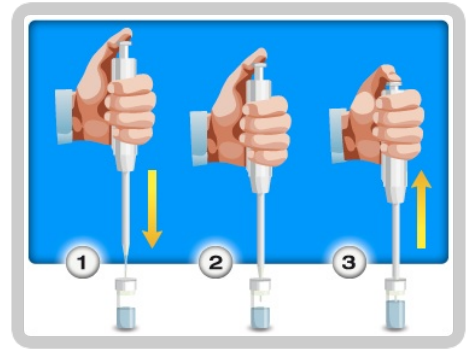


3. Add 30 µL of R2 to the cuvette without touching the tip in the liquid, R1 + sample. In case of contamination, replace the tip.

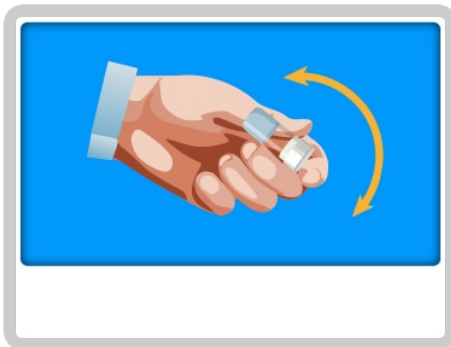


4. Gently shake the cuvette 2-3 times.




5. Select the cuvette to be read from the display. Place the cuvette in the cell marked with the blue light and press READ.

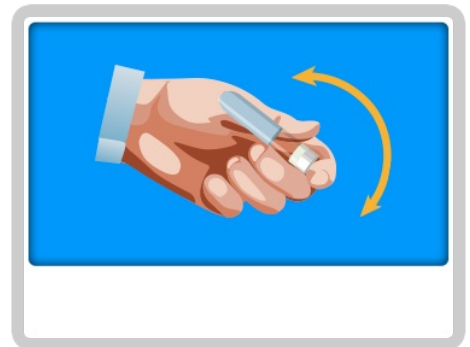


6. Homogenize the sample before collection.

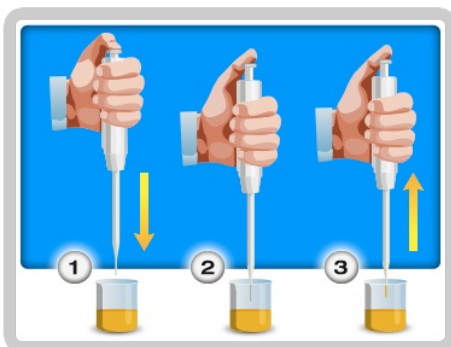


7. Draw the sample with the pipette 2-3 times and release it on blotting paper before collecting it for the test. Then collect 2.5 µL of sample.

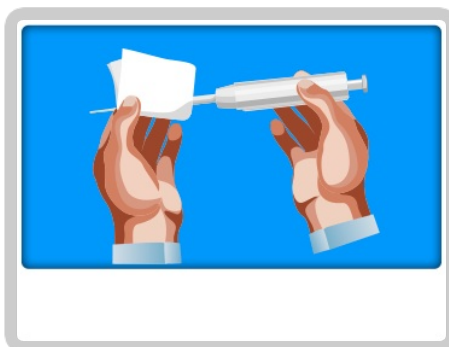

8. Carefully clean the outside of the pipette tip with blotting paper, avoiding contact between the extremity of the tip and the paper.

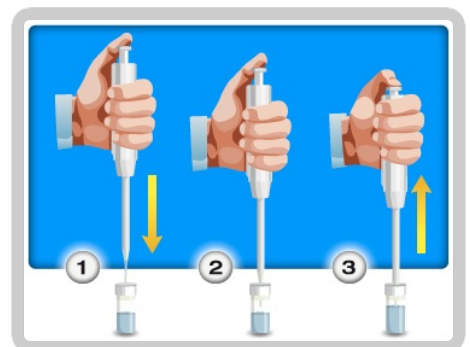

9. Place the sample in the cuvette. Keeping the tip immersed in reagent, press and release the piston of the pipette several times.

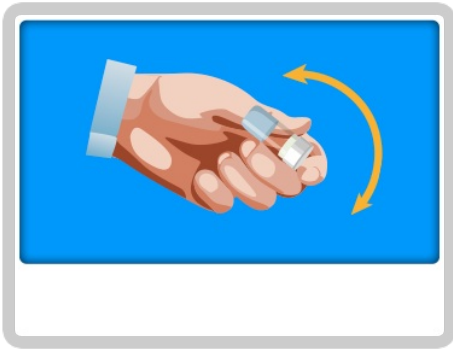

10. Gently shake the cuvette 2-3 times.



11. Place the cuvette in the cell marked with the blue light and press READ to perform the photometric reading.